

WEGO



CE₀₁₂₃ TÜV

Blood Collection Tube with Vacuum for Single Use



WEIGAO MEDICAL INTERNATIONAL CO., LTD.

ADD: No.1 Weigao Road, Hi-Tech Zone, Weihai, Shandong, China
TEL: +86 631 5660699 FAX: +86 631 5622563 P.C.: 264210
E-mail: info@weigaogroup.com exp@weigaogroup.com
Http://www.wegomedical.com/

This copyright belongs to Wego Medical International Co., Ltd. Our company reserves the right to investigate legal liability in case of infringement.

2024.2 EDITION

About WEGO Group

Established in 1988, with more than 30 years of dedication to medical devices and pharmaceuticals production, Wego continuously strives for excellence in developing and delivering quality products and services in healthcare. We focus on Clinical Nursing, Orthopedics, Blood Purification, IVD Supply, Wound Care, Surgery Consumables, Medical Imaging, Intervention, Medical Equipment, and Service. Based on the value of "Your health We care," we tirelessly improve our products, which are recognized and exported to over 150 countries and regions. WEGO's products are FDA-approved and are certified to CE, ISO, GMP, and IVDD.

Today, Wego's 30,000 employees across the world set our mission, making the world a better place by bringing life-changing health technologies and innovative medical system solutions to the people.






WG03-001-001 Fluoride Tubes(Blood Glucose)

| Reference Number | Tube Size (mm) | Volume (ml) | Glass/Plastic | Cap Colour | Pack/ Carton |
|------------------|----------------|-------------|---------------|------------|--------------|
| GF1307502 | 13x75 | 2.0 | G | GREY | 100/1800 |
| PF1207502 | 12x75 | 2.0 | P | GREY | 100/1800 |
| GF1307503 | 13x75 | 3.0 | G | GREY | 100/1800 |
| PF1207503 | 12x75 | 3.0 | P | GREY | 100/1800 |
| GF1310005 | 13x100 | 5.0 | G | GREY | 100/1200 |
| PF1210005 | 12x100 | 5.0 | P | GREY | 100/1200 |
| GF1310007 | 13x100 | 7.0 | G | GREY | 100/1200 |
| PF1210065 | 12x100 | 7.0 | P | GREY | 100/1200 |

■ Glucose tube with additive of potassium oxalate/sodium fluoride EDTA is used for test of blood coagulation mechanism.

■ Reference centrifugation speed:
300-3500 rpm for 5-8 mins

■ Additive status: Spray

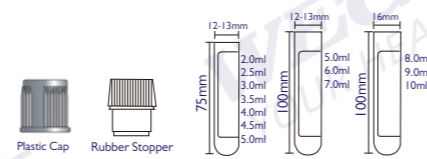


WG03-001-002 EDTA Tubes(Whole Blood)

| Reference Number | Tube Size (mm) | Volume (ml) | Glass/Plastic | Cap Colour | Pack/ Carton |
|------------------|----------------|-------------|---------------|------------|--------------|
| EDTA K2 | | | | | |
| GE1307522 | 13x75 | 2.0 | G | LAVENDER | 100/1800 |
| PE1207522 | 12x75 | 2.0 | P | LAVENDER | 100/1800 |
| GE1307523 | 13x75 | 3.0 | G | LAVENDER | 100/1800 |
| PE1207523 | 12x75 | 3.0 | P | LAVENDER | 100/1800 |
| GE1307525 | 13x75 | 5.0 | G | LAVENDER | 100/1800 |
| PE1210025 | 12x100 | 5.0 | P | LAVENDER | 100/1200 |
| EDTA K3 | | | | | |
| GE1307532 | 13x75 | 2.0 | G | LAVENDER | 100/1800 |
| PE1207532 | 12x75 | 2.0 | P | LAVENDER | 100/1800 |
| GE1307533 | 13x75 | 3.0 | G | LAVENDER | 100/1800 |
| PE1207533 | 12x75 | 3.0 | P | LAVENDER | 100/1800 |
| GE1307535 | 13x75 | 5.0 | G | LAVENDER | 100/1800 |
| PE1210035 | 12x100 | 5.0 | P | LAVENDER | 100/1200 |

■ EDTA tubes can be used on whole blood hematology determinations, blood thpe verification and equipment.

■ 1.8mg EDTA-K2 K3 per 1ml

■ Additive status: Spray

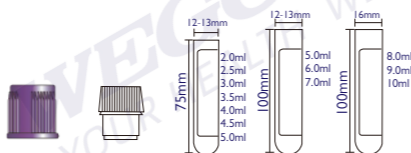


WG03-001-003 Heparin Tubes (Plasma)

| Reference Number | Tube Size (mm) | Volume (ml) | Glass/Plastic | Cap Colour | Pack/ Carton |
|------------------|----------------|-------------|---------------|------------|--------------|
| SODIUM HEPARIN | | | | | |
| GS130752 | 13x75 | 2.0 | G | GREEN | 100/1800 |
| PS120752 | 12x75 | 2.0 | P | GREEN | 100/1800 |
| GS130753 | 13x75 | 3.0 | G | GREEN | 100/1800 |
| PS120753 | 12x75 | 3.0 | P | GREEN | 100/1800 |
| GS131005 | 13x100 | 5.0 | G | GREEN | 100/1200 |
| PS121005 | 12x100 | 5.0 | P | GREEN | 100/1200 |
| LITHIUM HEPARIN | | | | | |
| GL130752 | 13x75 | 2.0 | G | GREEN | 100/1800 |
| PL120752 | 12x75 | 2.0 | P | GREEN | 100/1800 |
| GL130753 | 13x75 | 3.0 | G | GREEN | 100/1800 |
| PL120753 | 12x75 | 3.0 | P | GREEN | 100/1800 |
| GL131005 | 13x100 | 5.0 | G | GREEN | 100/1200 |
| PL121005 | 12x100 | 5.0 | P | GREEN | 100/1200 |

■ Plasma tube with Lithium Heparin, Sodium Heparin used in anti-coagulation not only for routine clinical biochemistry tests and emergency biochemistry tests but also for some test items in blood theology.

■ Reference centrifugation speed:
3000-3500 rpm for 5-8 mins

■ Additive status: spray

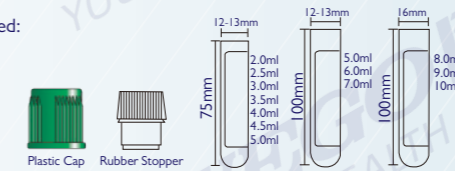


WG03-001-004 Sodium Citrate 1:4 Tubes (ESR)

| Reference Number | Tube Size (mm) | Volume (ml) | Glass/Plastic | Cap Colour | Pack/ Carton |
|------------------|----------------|-------------|---------------|------------|--------------|
| GN1307516 | 13x75 | 1.6 | G | BLACK | 100/1800 |
| PN1207516 | 12x75 | 1.6 | P | BLACK | 100/1800 |
| GN1307524 | 13x75 | 2.4 | G | BLACK | 100/1800 |
| PN1207524 | 12x75 | 2.4 | P | BLACK | 100/1800 |
| GN0812016 | 8x120 | 1.6 | G | BLACK | 100/1200 |
| GN0812012 | 8x120 | 1.28 | G | BLACK | 100/1200 |

■ Sodium Citrate 1:4 used with 3.2%(0.109mol/L) sodium citrate for anti coagulation and ratio of anticoagulant and blood is 1:4

■ Additive status: liquid

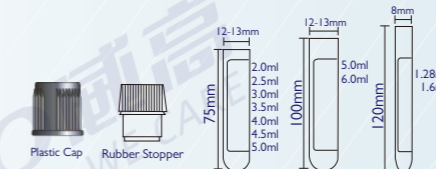




WG03-001-005 Plain Tubes (Serum)

| Reference Number | Tube Size (mm) | Volume (ml) | Glass/Plastic | Cap Colour | Pack/ Carton |
|------------------|----------------|-------------|---------------|------------|--------------|
| GPI307502 | 13x75 | 2.0 | G | RED | 100/1800 |
| PPI207502 | 12x75 | 2.0 | P | RED | 100/1800 |
| GPI307503 | 13x75 | 3.0 | G | RED | 100/1800 |
| PPI207503 | 12x75 | 3.0 | P | RED | 100/1800 |
| PPI307505 | 13x75 | 5.0 | G | RED | 100/1800 |
| GPI310005 | 13x100 | 5.0 | G | RED | 100/1200 |
| PPI210005 | 12x100 | 5.0 | P | RED | 100/1200 |
| GPI310007 | 13x100 | 7.0 | G | RED | 100/1200 |
| PPI210065 | 12x100 | 7.0 | P | RED | 100/1200 |
| GPI610010 | 16x100 | 10.0 | G | RED | 100/1200 |
| PPI610010 | 16x100 | 10.0 | P | RED | 100/1200 |


- Serum tube can be used in collecting blood sample in clinical bichemistry and immunology.
- Reference centrifugation speed: 300-3500rpm
- Reference clotting time:
No additive 40-60 mins, Activator 10 mins.
- Additive status: Spray

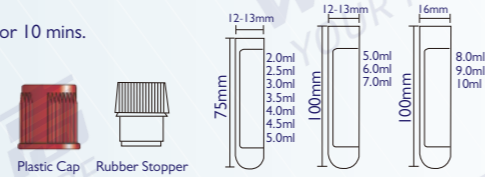

WG03-001-006 GEL Tubes (Serum Separator)

| Reference Number | Tube Size (mm) | Volume (ml) | Glass/Plastic | Cap Colour | Pack/ Carton |
|------------------|----------------|-------------|---------------|------------|--------------|
| GGI307503 | 13x75 | 3.0 | G | YELLOW | 100/1800 |
| PGI207503 | 12x75 | 3.0 | P | YELLOW | 100/1800 |
| GGI310005 | 13x100 | 5.0 | G | YELLOW | 100/1200 |
| PGI210005 | 12x100 | 5.0 | P | YELLOW | 100/1200 |
| GGI610007 | 16x100 | 7.0 | G | YELLOW | 100/1200 |
| PGI610007 | 16x100 | 7.0 | P | YELLOW | 100/1200 |
| GGI610009 | 16x100 | 9.0 | G | YELLOW | 100/1200 |
| PGI610009 | 16x100 | 8.0 | P | YELLOW | 100/1200 |

- GEL can be used in separating serum and plasma, pre-filled for quick serum measurement and immunology test.
- Suggested centrifugation speed:
3000-3500rpm for 5-8MINS
- Additive status: GEL


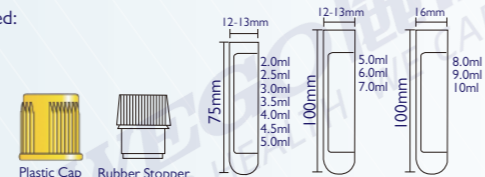


WG03-001-007 Sodium Citrate 1:9 Tubes (Coagulation)

| Reference Number | Tube Size (mm) | Volume (ml) | Glass/Plastic | Cap Colour | Pack/ Carton |
|------------------|----------------|-------------|---------------|------------|--------------|
| GGI307503 | 13x75 | 1.8 | G | BLUE | 100/1800 |
| PNI207518 | 12x75 | 1.8 | P | BLUE | 100/1800 |
| GNI307527 | 13x75 | 2.7 | G | BLUE | 100/1800 |
| PNI207527 | 12x75 | 2.7 | P | BLUE | 100/1800 |
| GNI307545 | 13x75 | 4.5 | G | BLUE | 100/1800 |
| PNI207545 | 12x75 | 4.5 | P | BLUE | 100/1800 |
| PNI210045 | 12x100 | 4.5 | P | BLUE | 100/1200 |

- Sodium Citrate 1:9 with 3.8% (0.129mol/L) sodium citrate as anticoagulant used for coagulation test and ratio of anticoagulant and blood is 1:9

- Additive status: liquid

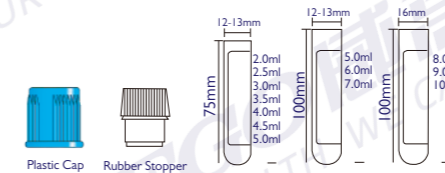

WG03-001-008 Sodium Citrate 1:9 Tubes (Double Wall)

| Reference Number | Tube Size (mm) | Volume (ml) | Glass/Plastic | Cap Colour | Pack/ Carton |
|------------------|----------------|-------------|---------------|------------|--------------|
| PNI207518 | 12x75 | 1.8 | P | BLUE | 100/1800 |
| PNI207527 | 12x75 | 2.7 | P | BLUE | 100/1800 |

- Sodium Citrate 1:9 used with 3.2% (0.109mol/L) sodium citrate for anti coagulation and Ratio of anticagulant and blood is 1:9

- Additive status: liquid



External Tube
12X75mm PET
Vacuum retention
Consistent outer dimension

Internal Tube
Smaller Polypropylene
Minimal Platelet activation
Good liquid barrier

Aluminum-plastic bag:
Prevents additive water from evaporating and keeps solution concentration stable for a long time.

WG03-001-009 Blood Collection Needles

| Reference Number | Needle Size | Length (mm) | Reference Colour | Type | Inner Box/ Carton |
|------------------|-------------|-------------|------------------|------------------------------------|-------------------|
| VNP20009 | 18G | 38 | PINK | BUTTERFLY WINGS WITH TUBE/PEN LIKE | 100/5000 |
| VNP20100 | 20G | 25 | YELLOW | BUTTERFLY WINGS WITH TUBE/PEN LIKE | 100/5000 |
| VNP20112 | 20G | 38 | YELLOW | BUTTERFLY WINGS WITH TUBE/PEN LIKE | 100/5000 |
| VNP21100 | 21G | 25 | GREEN | BUTTERFLY WINGS WITH TUBE/PEN LIKE | 100/5000 |
| VNP21112 | 21G | 38 | GREEN | BUTTERFLY WINGS WITH TUBE/PEN LIKE | 100/5000 |
| VNP22100 | 22G | 25 | BLACK | BUTTERFLY WINGS WITH TUBE/PEN LIKE | 100/5000 |
| VNP22112 | 22G | 38 | BLACK | BUTTERFLY WINGS WITH TUBE/PEN LIKE | 100/5000 |
| VNP22113 | 23G | 25 | NAVY BLUE | BUTTERFLY WINGS WITH TUBE/PEN LIKE | 100/5000 |
| VNH20000 | | | | PLASTIC NEEDLE HOLDER | 100/2000 |



- Vacuum blood collection needle and holder are used with vacuum tubes to collect the blood, the needle size marked with different colors in 20G, 21G and 22G.

- Note: Please use the needle by the professional user and under correct performance to avoid the needlestick injury.